

New External Fixators for Treatment of Pelvis and Acetabulum Fractures

K. Frydryšek, L. Pleva, J. Jořenek, V. Ječmínek, R. Klučka, M. Sivera

Abstract— At first, the doctors mentioned their own medical experience with treatment of complex pelvic injury in patients with polytrauma and give reasons for necessity of early stabilization of pelvic fractures by means of external fixation, especially with continuous hemorrhage into lesser pelvis region and the retroperitoneum. Afterwards they used damage control surgery methods including selective embolization. However, this article is focused also on the design of external fixators applied in traumatology and orthopaedics (i.e. skills of engineers). These fixators can be used in the treatment of open and unstable (i.e. complicated) fractures of pelvis and its acetabulum. Two versions (i.e. old and new) are compared. Numerical modelling (i.e. Finite Element Method), together with CAD modelling, experiments, material engineering, and nanotechnology are presented as a support for developing of a new design of external fixators.

Keywords—traumatology, pelvis, complex injuries, polytrauma, acetabulum, fractures, design, biomechanics, numerical modeling

I. INTRODUCTION

INCREASING number of high-energy injuries brings increase in number of complex injuries of the pelvis, where apart from fractures of the pelvic girdle also arteries, nerves, soft tissues and pelvic intraperitoneal and retroperitoneal organs are injured. The most severe complication of these injuries consists in extensive hemorrhage, mainly from injured skeleton, a presacral

Assoc. Prof. M.Sc. Karel FRYDRÝŠEK, Ph.D., ING-PAED IGIP, Department of Mechanics of Materials, Faculty of Mechanical Engineering, VŠB – Technical University of Ostrava, 17. listopadu 15/2172, 708 33 Ostrava, Czech Republic (phone: +420 597323495, e-mail: karel.frydrysek@vsb.cz).

Assoc. prof., M.D. Leopold PLEVA, Ph.D., Trauma Centre, University Hospital in Ostrava, 17. listopadu 1790, 708 52, Ostrava, Czech Republic (e-mail: leopold.pleva@fno.cz).

M.Sc. Jaroslav JOŘENEK; Department of Mechanics of Materials; Faculty of Mechanical Engineering, VŠB - Technical University of Ostrava, 17. listopadu 15/2172, 708 33 Ostrava, Czech Republic (e-mail: jaroslav.jorenek.st@vsb.cz).

M.D. Vladimír JEČMÍNEK, Ph.D., Trauma Centre, University Hospital in Ostrava, 17. listopadu 1790, 708 52, Ostrava, Czech Republic (e-mail: vladimir.jecminek@fno.cz).

M.Sc. Richard KLUČKA, Department of Mechanics of Materials, Faculty of Mechanical Engineering, VŠB – Technical University of Ostrava, 17. listopadu 15/2172, 708 33 Ostrava, Czech Republic (e-mail: richard.klucka@seznam.cz).

M.Sc. Milan SIVERA, Department of Mechanics of Materials, Faculty of Mechanical Engineering, VŠB – Technical University of Ostrava, 17. listopadu 15/2172, 708 33 Ostrava, Czech Republic (e-mail: sivera.milan@email.cz).

and paravesical vascular plexes that can directly threaten life of the injured child by hemorrhagic traumatic shock.

Diagnostic methods, apart from RTG pelvis, are ultrasonography, computer tomography and computed angiography, see [1].

The basis for the treatment of instable pelvic fractures consists of pelvic skeleton stabilization, which in the urgent stage is ensured by application of a pelvic clamp with subsequent application of external fixator, see [1] – [4], [7] – [12] and Fig. 1.



Fig. 1 Complex pelvis fracture treated with external fixator (Trauma Centre, University Hospital in Ostrava, Ostrava, Czech Republic)

In case of continuous hemorrhage, we perform urgent AG with surgical treatment of injured arteries or their selective embolization, see [5]. In extensive devastating injuries we do not hesitate to perform tamponade of the pelvis with possible bilateral ligation of a. iliaca interna, see [6].

II. EXTERNAL FIXATORS

However, this article reports about the designing of external fixators applied in traumatology and orthopaedics. This work was performed by VŠB – Technical University of Ostrava together with University Hospital in Ostrava and company MEDIN a.s. (Czech Republic), see web page [9] and [10] (i.e. work of the project External Fixation, see Fig. 2 and 3).

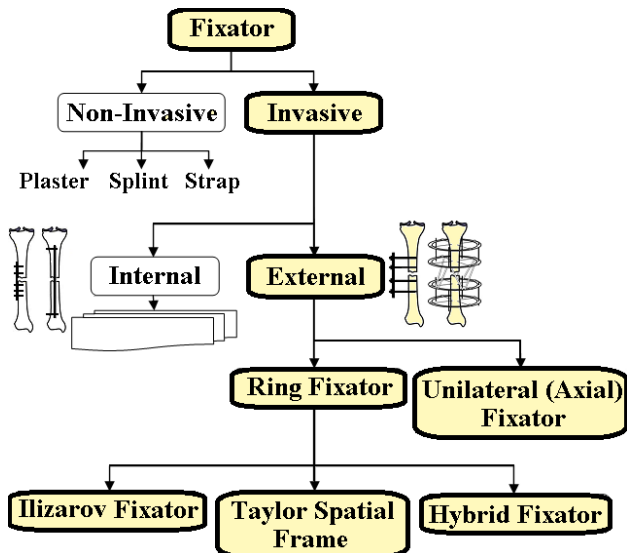


Fig. 2 Focus of our project “External Fixation”, see web page [9].



Fig. 3 Application of external fixator (treatment of a dog, treatment of a human - experiments in the laboratory at VSB – Technical university of Ostrava)

External fixation, see Fig. 2 and 3, is a surgical treatment usually used to set bone fractures in which a cast (plaster) would not allow proper alignment of the fracture. In this kind of treatment, holes are drilled into uninjured areas of bones around the fracture and special bolts or wires are screwed into the holes. Outside the body, rods and curved pieces of metal with special joints (bracket) connect the bolts to make a stiff support. The complicated fracture, see Fig. 3 and 4, can be set in the proper anatomical configuration, see ref. [1] – [16].

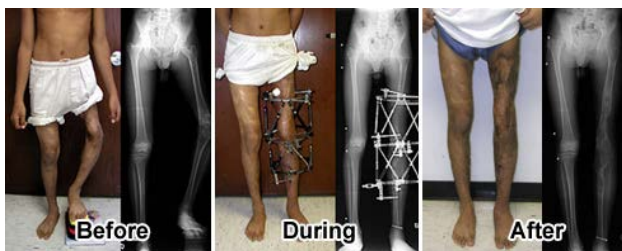


Fig. 4 Application of external fixator (consequences of poliomyelitis, foot deformities, source internet)

III. FIXATORS FOR TREATMENT OF PELVIS AND ACETABULAR FRACTURES

This article is focused on the external fixators intended for pelvis. These fixators can be applied in the treatment of open and unstable (i.e. complicated) fractures of pelvis and its acetabulum, for example see Fig. 5 and a radiograph presented in Fig. 6.

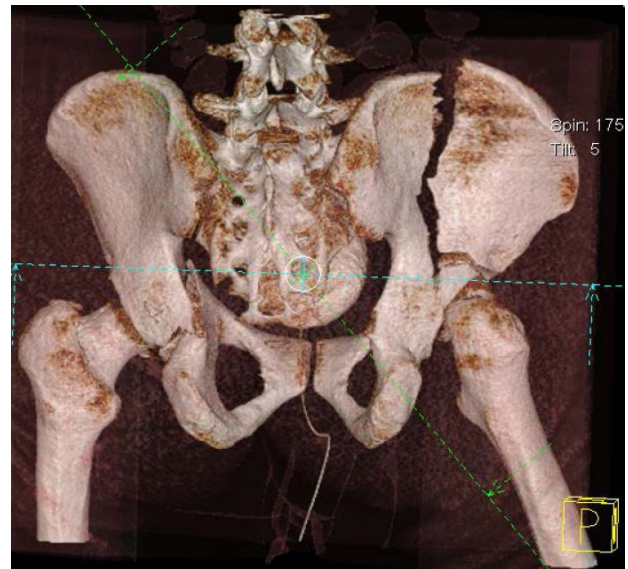


Fig. 5 Examples of pelvis fracture

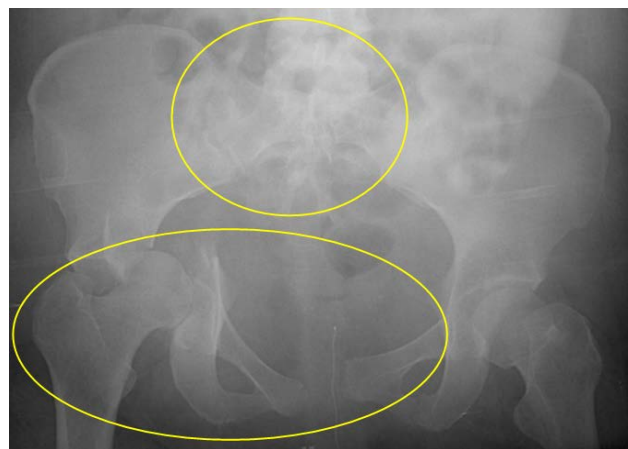


Fig. 6 Fracture of pelvis and its acetabulum (anteroposterior radiograph - transverse with posterior wall acetabular fracture)

Acetabular fractures, see Fig. 6 and 7, either occur with high-energy trauma (e.g. automobile collisions, falls, etc.) or as an insufficiency fracture. In younger patients, there is almost always significant trauma, and commonly associated injuries, when an acetabular fracture occurs. In elderly patients, acetabular fractures can occur due to bone weakened (i.e. consequences of osteoporosis, periprosthetic fractures etc.).



Fig. 7 Examples of acetabular fractures

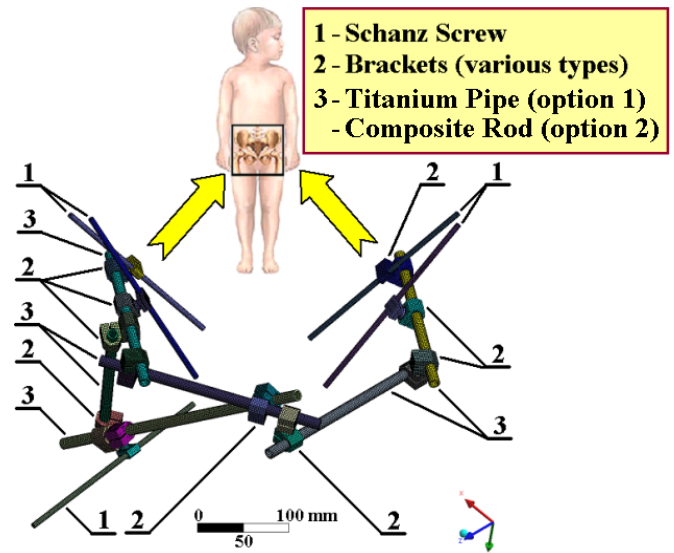


Fig. 8 Application of external fixator for treatment of pelvis and its acetabulum

IV. NEW REQUIREMENTS FOR DESIGNING EXTERNAL FIXATORS

At the VŠB – Technical University, two designs of external fixators intended for treatment of pelvis and acetabulum fractures was designed and tested (i.e. an old version noted as “Option 1” and a new and modern version noted as “Option 2”), see Fig. 8 and ref. [7] and [12].

DEMANDS:	BENEFITS AND EXPLANATION:	GOALS:
Outer parts of fixators must be x-ray invisible (i.e. low x-ray absorption):	Easy to see fracture; reducing radiation exposure for patients and surgeons; shortening the operating time.	New smart materials (mostly not metal)
Antibacterial protection:	Application of nanoadditives containing selected metal-based nanoparticles on the surface of the outer parts of the fixators may allow for growth inhibition of several pathogens and thus prevent or reduce possible infection. Antibacterial protection gives products an added level of protection against damaging microbes such as, bacteria, mould and mildew that can cause cross-contamination and product deterioration. Antibacterial nanotechnology, combined with regular cleaning practices, helps to improve hygiene standards and provides extra protection wherever it is used. Antibacterial protection based on the nanotechnology was tested in the laboratory conditions.	
Material Engineering:	Material proposition and material tests; proper mechanical properties.	
Ecological perspective:	Easy to recycle.	New design (structure)
Weight optimization:	To avoid the overloading of limbs fixed by external construction. This is based on the application of numerical methods and experiments too.	
Patient's comfort:	Reducing the time of the surgical operation and reducing the overall cost. Technical aesthetics of fixators also have impacts on the psyche of the patients (i.e. "friendly-looking design of fixators"). For example, patients usually have better feelings, easier motion and physiotherapy with fixators made up from lighter composites (reinforced plastics) than heavier metals.	
Easy to assembly:		Numerical modelling (FEM, SBRA Method) and experiments
Proper mechanical properties:	Stiffness of the whole system of fixators, fatigue testing, etc. are based on laboratory testing of new smart materials.	
Measuring of the real loadings:	During the patient's treatment measurements of the real loadings and stiffness of the external fixators (laboratory measurement and measurement in vivo - painlessly) and data processing are needed. This is based on strain gauge measurement and applied statistics and the Simulation-Based Reliability Assessment (SBRA) Method, see [17] – [26]. This type of measuring and processing in vivo has never been applied before to the solution of problems of external fixators.	

Table I New ways for designing external fixators applied in treatment of open and unstable fractures

Scientific and technical developments, together with medical care and practice and engineering bring new demands for designs of external fixators. These demands are presented in Table I.

Two versions of external fixators (“Option 1” and “Option 2”) were solved, see Fig. 8.

V. EXPERIMENTS

The “Option 1” is fully metallic (i.e. the old design which does not satisfy the new demands presented in Table I).

On the contrary, the “Option 2” is partly metallic (i.e. the new design which satisfies the new demands presented in Table I). There are composite rods made of carbon fibres which are x-ray invisible, see Fig. 8.

The new types of external fixators for treatment of fractures of pelvis and its acetabulum were tested in the laboratory at the VŠB – Technical University of Ostrava (Ostrava, Czech Republic), see [15] and Fig. 9.



Fig. 9 Measurements in the laboratory

The experiments were focused mainly on the stiffness and reliability for the whole system of the fixator and pelvis interaction (i.e. pulling the hip bone outwards from acetabulum after the reposition of pelvis fragments – axial tensile force 100 N in Schanz screw).

VI. NUMERICAL MODELLING

The CAD models of external fixators (i.e. “Option 1” and “Option 2”), see Fig. 8), were imported into the Finite Element (FE) software Ansys Workbench. In this software, the FE meshes were created, see Fig. 10 and 11.

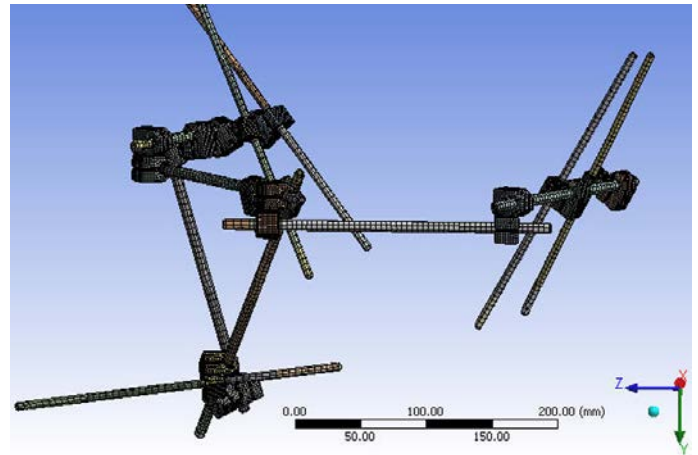


Fig. 10 FE mesh for external fixator (whole structure)

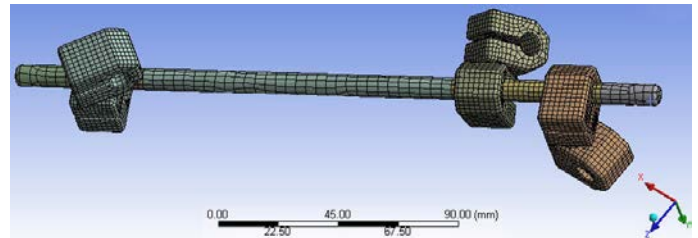


Fig. 11 FE mesh for external fixator (detail)

The basic information about the boundary conditions is presented in Fig. 12. There are defined mechanical contacts with friction between the brackets and titanium pipes (“Option 1”) or between the brackets and composite rods (“Option 2”) and between brackets and Schanz screws.

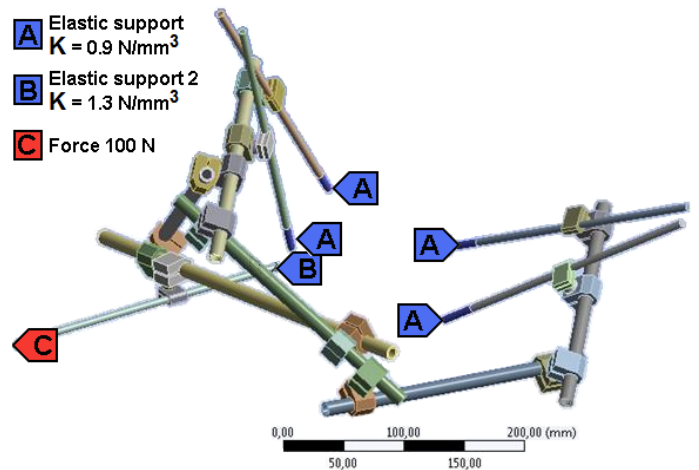


Fig. 12 FE model (boundary conditions) of external fixator for pelvis and its acetabulum

Schanz screws are embedded in pelvis and its acetabulum in drilled holes. Their attachments are modelled by elastic supports (i.e. by Winkler's foundation, see point “A” and “B” in Fig. 12). The elastic support (defined via modulus of foundation $K \text{ /Nm}^{-3}$), see Fig. 12) is applied in the radial and axial direction on the surface parts of Schanz screws. This is quite good and popular simplification of the real complicated interaction between screw and bone, see [16], [19] and

[27] – [29].

Loading force 100 N (see point “C” in Fig. 12) is explained in the end of Chapter V.

From the results, for example see Fig. 13, 14, Table II and [16], is evident very important improvement of the new design (i.e. the new design “Option 2” is better than the design “Option 1”). In the Table II, the symbols “+” or “-” mean the positive or negative aspects in designing.

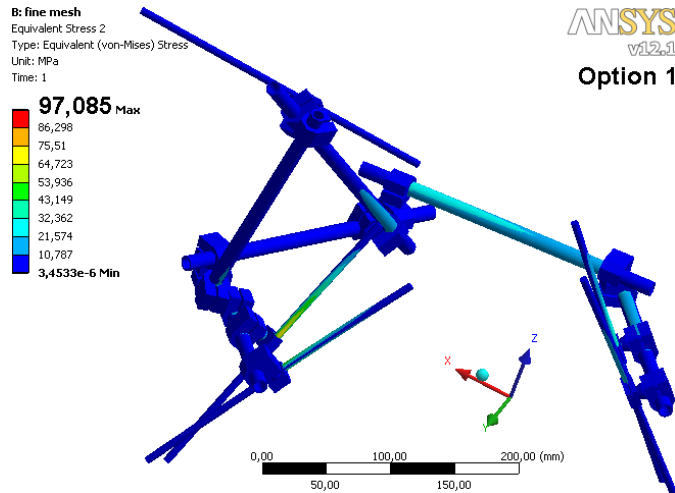


Fig. 13 “Option 1” - FE modelling of external fixator for pelvis and acetabulum (equivalent stresses for tensile loading 100 N)

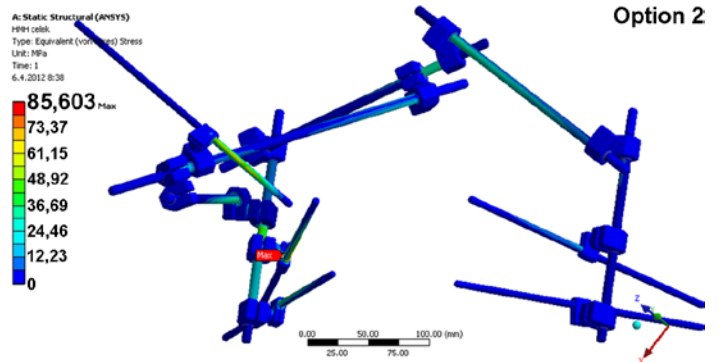


Fig. 14 “Option 2” - FE modelling of external fixator for pelvis and acetabulum (equivalent stresses for tensile loading 100 N)

VII. CONCLUSION

According to the results presented in Table II (i.e. comparing of the new design with the old one), the improvements in the designing of external fixators for treatment of pelvis and acetabulum fractures are evident.

The results of experiments fit well with numerical modelling.

VŠB - Technical University of Ostrava together with University Hospital of Ostrava and Trauma Hospital of Brno are now in the middle of a process creating new designs for external fixators. Hence, they are in cooperation with the Czech producers MEDIN Nové Město na Moravě (Czech Republic). Therefore, all results could not be published in this paper due to confidentiality reasons.

Report about the new ways to design of external fixator for the treatment of fractures of pelvis and its acetabulum, based on the results of previous research, was presented. Hence, the new designs and materials of fixators will satisfy the ambitious demands of modern traumatology, surgery and economics.

ACKNOWLEDGMENT

This work has been supported by the Czech projects MPO FR-T13/818 “External Fixation” and by Czech project TA03010804 “Osteosynthesis of Leg and Arm Fractures” and by Czech-Slovak project 7AMB12SK123 resp. SK-CZ-0028 “Theory and Practice of Structures on Elastic Foundations”.

REFERENCES

- [1] J. Chmelová, M. Šír, V. Ječmínek, CT-Guided Percutaneous Fixation of Pelvic Fractures Case Reports, *Biomed. Papers*, 149 (1), pp. 177–181 (2005)
- [2] K. D. Johnson, A. Cadambi, B. Seibert, Incidence of adult respiratory distress syndrome in patients with multiple musculoskeletal injuries: effect of early stabilization of fractures, *J. Trauma*, 1985, 25 (5), 375.
- [3] R. Tomaszewski, W. Bijata, P. Starzak, J. Bohosiewicz, Two-stage treatment of an unstable fracture of the pelvic ring in a 4-year-old child, *Rocznik Dziecięcej Chirurgii Urazowej*, ISSN 1507-5931, 2004, 8 (XXXII), 123, Poland.
- [4] V. Ječmínek, P. Prusenovský, R. Vronský, Complex injury of the pelvis in Children, *Rocznik Dziecięcej Chirurgii Urazowej*, ISSN 1507-5931, 2005, 9 (XXXIII), 123, Poland.
- [5] M. J. Bosse, J. F. Kellam, Orthopedic Management Decisions in the Multiple Trauma Patient, in: *Skeletal Trauma*, (ed.) Browner B.D. Jupiter J., Levine A. et al. Philadelphia, USA, 2003.

ATTRIBUTES:	OPTION 1:	OPTION 2:
Design:	⊖ old	⊕ new
Material:	⊖ titanium, stainless steel	⊕ carbon fibre, titanium, stainless steel
Added antibacterial protection:	⊖ no	⊕ yes
X-ray invisible:	⊖ no	⊕ partly yes
Weight of external fixator	⊖	⊕ decreasing
Stiffness of external fixator:	⊖	⊕ increasing
Maximum von Mises stresses /MPa/:	⊖ 97.1, see Fig. 17	⊕ 85.6 – decreasing, see Fig. 18
Maximum total deformation /mm/:	⊖ 5.74	⊕ 4.32 - decreasing
Patient comforts:	⊖	⊕ improvement
Reliability assessment	⊖	⊕ improvement
Easy to assembly:	the same	

Table II Results comparing – external fixator for pelvis and its acetabulum (designs “Option 1” and “option 2”)

- [6] H. C. Pape, P. Giannoudis, C. Krettek, The timing of fracture treatment in polytrauma patients, relevance of damage control orthopedic surgery. *Am. J. Surg.*, 2002, 183 (6), 622.
- [7] K. Frydryšek, P. Košťál, K. Barabaszová, J. Kukutschová, New ways for designing external fixators applied in treatment of open and unstable Fractures, *J. World Academy of Science, Engineering and Technology*, ISSN 2010-376X (print version) ISSN 2010-3778 (electronic version), vol. 7, issue 76, 2011, pp. 639–644.
- [8] L. Pleva, *External fixator for treatment of acetabulum fractures*, final report of the project IGA MZ ČR, reg. č. 3522-4, written in Czech language, FNŠP – Ostrava-Poruba, 1999, Czech Republic, pp. 1–77.
- [9] <http://aplmech.vsb.cz/zevni-fixace/>
- [10] <http://www.akutne.cz/res/publikace/damage-control-komplexniho-poraneni-panve-ruber-v.pdf>
- [11] D. Seligson, C. Mauffrey, C. S. Roberts editors, *External fixation in orthopedic traumatology*, London, Springer, 2012, ISBN 978-1-4471-2199-2 (hard) 978-1-4471-2197-8 (e-book), pp. 1-228.
- [12] K. Frydryšek, J. Jořenek, P. Košťál, V. Ječmínek, L. Pleva, K. Barabaszová, I. Ružiak, External Fixators for Treatment of Complicated Pelvis Fractures, In: *World Academy of Science, Engineering and Technology*, pISSN 2012-376X, eISSN 2012-3778, issue 69, Singapore, 2012, pp. 676-681.
- [13] K. Frydryšek, L. Pleva, M. Janečka, R. Klučka, M. Sivera, J. Jořenek, Report about the New External Fixator for Treatment of Pelvis and Acetabulum Fractures, In: *Latest Advances in Biology, Environment and Ecology*, ISBN 978-1-61804-097-8, North Atlantic University Union, WSEAS Press, Iasi, Romania, 2012, pp.144-147.
- [14] K. Frydryšek, L. Pleva, O. Učeň, T. Kubín, J. Rojíček, M. Šír, R. Madeja, Report about the New External Fixator for Treatment of Complicated Limb Fractures, In: *Latest Advances in Biology, Environment and Ecology*, ISBN 978-1-61804-097-8, North Atlantic University Union, WSEAS Press, Iasi, Romania, 2012, pp.148-151.
- [15] M. Janečka, *Výzkum a vývoj zevního fixátoru na pánev (acetabulum), včetně experimentálního měření a počítačového modelování*, thesis of Ph.D. work, VŠB – Technical University of Ostrava, Ostrava, Czech Republic, pp. 1–17, written in Czech language.
- [16] J. Jořenek, *Biomechanics – External fixator for pelvis and acetabulum (Biomechanika – Externí fixátor pro pelvis a acetabulum)*, diploma thesis, VŠB – Technical University of Ostrava, Ostrava, Czech Republic, pp. 1–68, written in Czech language.
- [17] P. Marek, J. Brozzetti, M. Guštar, P. Tikalsky, *Probabilistic Assessment of Structures Using Monte Carlo Simulation Background, Exercises and Software*, (2nd extended edition), ISBN 80-86246-19-1, ITAM CAS, Prague, Czech Republic, 2003.
- [18] P. Marek, M. Guštar, T. Anagnos, *Simulation-Based Reliability Assessment For Structural Engineers*, CRC Press, Boca Raton, USA, ISBN 0-8493-8286-6, 1995.
- [19] K. Frydryšek, *Probabilistic Calculations in Mechanics I (Pravděpodobnostní výpočty v mechanice I)*, ISBN: 978-80-248-2314-0, VŠB - Technical University of Ostrava, 2010, pp. 1–149 (written in Czech language)
- [20] Z. Kala, Sensitivity Analysis of Steel Plane Frames with Initial Imperfections, in *Engineering Structures*, vol.33, no.8, 2011, pp. 2342-2349.
- [21] K. Frydryšek, Probabilistic Approach Applied in the Design of Machine Parts and Structures, In: *Recent Researches in Engineering and Automatic Control*, ISBN 978-1-61804-057-2, North Atlantic University Union, WSEAS Press, Puerto De La Cruz, Tenerife, Spain, 2011, pp.30-37.
- [22] K. Frydryšek, I. Wandrol, P. Kalenda, Report about the Probabilistic Approaches Applied in Mechanics of Continental Plates, In: *Mathematical Models and Methods in Modern Science*, vol. 3, ISBN 978-1-61804-106-7, ISSN 2227-4588, WSEAS Press, Porto, Portugal, 2012, pp.146-149.
- [23] J. Gottvald, Z. Kala, Variance-Based Sensitivity Analysis of Tangential Digging Forces of the Bucket Wheel Excavator SchRs 1320, In: *Recent Researches in Engineering and Automatic Control*, ISBN 978-1-61804-057-2, North Atlantic University Union, WSEAS Press, Puerto De La Cruz, Tenerife, Spain, 2011, pp.204-209.
- [24] J. Pokorný, K. Frydryšek, Horst Gondek, Meaning of Existence of Hot Gas Layer for Determination of the Fire Plume Centreline Temperature, *International Journal of Mathematical Models and Methods in Applied Sciences*, North Atlantic University Union, ISSN: 1998-0140, Issue 1, Volume 7, 2013, pp. 47-54, <http://www.naun.org/multimedia/NAUN/m3as/16-566.pdf>
- [25] K. Frydryšek, *Monte Carlo Approach Applied in the Design of Machine Parts and Structures*, International Journal of Mechanics, North Atlantic University Union, ISSN: 1998-4448, Issue 4, Volume 6, 2012, pp. 222-229, <http://www.naun.org/multimedia/NAUN/mechanics/16-574.pdf>
- [26] K. Frydryšek, I. Wandrol, P. Kalenda, Application of SBRA Method in Mechanics of Continental Plates, International Journal of Mechanics, North Atlantic University Union, ISSN: 1998-4448, Issue 4, Volume 6, 2012, pp. 230-237, <http://www.naun.org/multimedia/NAUN/mechanics/16-581.pdf>
- [27] K. Frydryšek, *Beams and Frames on Elastic Foundation 1 (Nosníky a rámy na pružném podkladu 1)*, Faculty of Mechanical Engineering, VŠB - Technical University of Ostrava, ISBN 80-248-1244-4, Ostrava, Czech Republic, 2006, pp.463, written in Czech language.
- [28] K. Frydryšek, R. Jančo, at all, *Beams and Frames on Elastic Foundation 2 (Nosníky a rámy na pružném podkladu 2)*, Faculty of Mechanical Engineering, VŠB - Technical University of Ostrava, ISBN 978-80-248-1743-9, Ostrava, Czech Republic, 2008, pp.516, written in Czech language.
- [29] K. Frydryšek, M. Nikodým, at all, *Beams and Frames on Elastic Foundation 3*, ISBN 978-80-248-2257-0, VŠB – Technical University of Ostrava, Ostrava, Czech Republic, 2010, pp.611., written in English and Czech languages.

Assoc. Prof. M.Sc. Karel FRYDRÝŠEK, Ph.D., ING-PAED IGIP (Department of Mechanics of Materials, Faculty of Mechanical Engineering, VŠB – Technical University of Ostrava, Ostrava, Czech Republic) - born in June 27th 1972, married, one daughter.

Study: M.Sc. - 1995, Ph.D. - 1999, Assoc. Prof. - 2009 in the branch of "Applied Mechanics" all at the Faculty of Mechanical Engineering VŠB – Technical University of Ostrava. He also studied pedagogy in the branch of "Academic Pedagogy for Teachers-Engineers According to the European Standards IGIP" at the Centre for Study of Academic Teaching in the Prague - 2003.

Scientific-research activities and cooperation with industry: Theory and practice of FEM and other numerical methods, strength and elasticity, plasticity, material tests, fatigue, thermal stresses, creep, comparing of experiments and calculations, stress-strain analyses in bodies, proposition of testing machines and its parts, rock mechanics, geomechanics, mechanics of composites and structures on elastic foundation. He has a rich cooperation with industry (automotive industry, railway industry, civil engineering, mining, metallurgy, forming, casting, heat technology, steel structures, pipe systems, biomechanics etc.). In the last years, he is focused on probabilistic reliability assessment (SBRA Method applications) and biomechanics (problems of design of external & internal fixators for treatment of open and unstable fractures in traumatology and orthopaedics).

Assoc. prof., M.D. Leopold PLEVA, Ph.D., Head Physician, Trauma Centre, University Hospital in Ostrava, 17. listopadu 1790, 708 52, Ostrava, Czech Republic (e-mail: leopold.pleva@fno.cz).

Under the leadership of Assoc. prof. Leopold Pleva, the Trauma Centre currently draws on significant traditions by introducing new operating methods in polytrauma, which are concentrated in the Trauma Center from the whole North-Moravian region. The scientific research activity focuses on solution of state research tasks, where the physicians of the Trauma Center are successful solvers of new therapeutic methods.

M.Sc. Jaroslav JOŘENEK; Ph.D. student in the branch of "Applied Mechanics", Department of Mechanics of Materials; Faculty of Mechanical Engineering, VŠB - Technical University of Ostrava, 17. listopadu 15/2172, 708 33 Ostrava, Czech Republic (e-mail: jaroslav.jorenek.st@vsb.cz).

M.D. Vladimír JEČMÍNEK, Ph.D., Trauma Centre, University Hospital in Ostrava, 17. listopadu 1790, 708 52, Ostrava, Czech Republic (e-mail: vladimir.jecminek@fno.cz).

M.Sc. Richard KLUČKA; Ph.D. student in the branch of “Applied Mechanics”, Department of Mechanics of Materials, Faculty of Mechanical Engineering, VŠB – Technical University of Ostrava, 17. listopadu 15/2172, 708 33 Ostrava, Czech Republic (e-mail: richard.klucka@seznam.cz).

M.Sc. Milan SIVERA; Ph.D. student in the branch of “Applied Mechanics”, Department of Mechanics of Materials, Faculty of Mechanical Engineering, VŠB – Technical University of Ostrava, 17. listopadu 15/2172, 708 33 Ostrava, Czech Republic (e-mail: sivera.milan@email.cz).